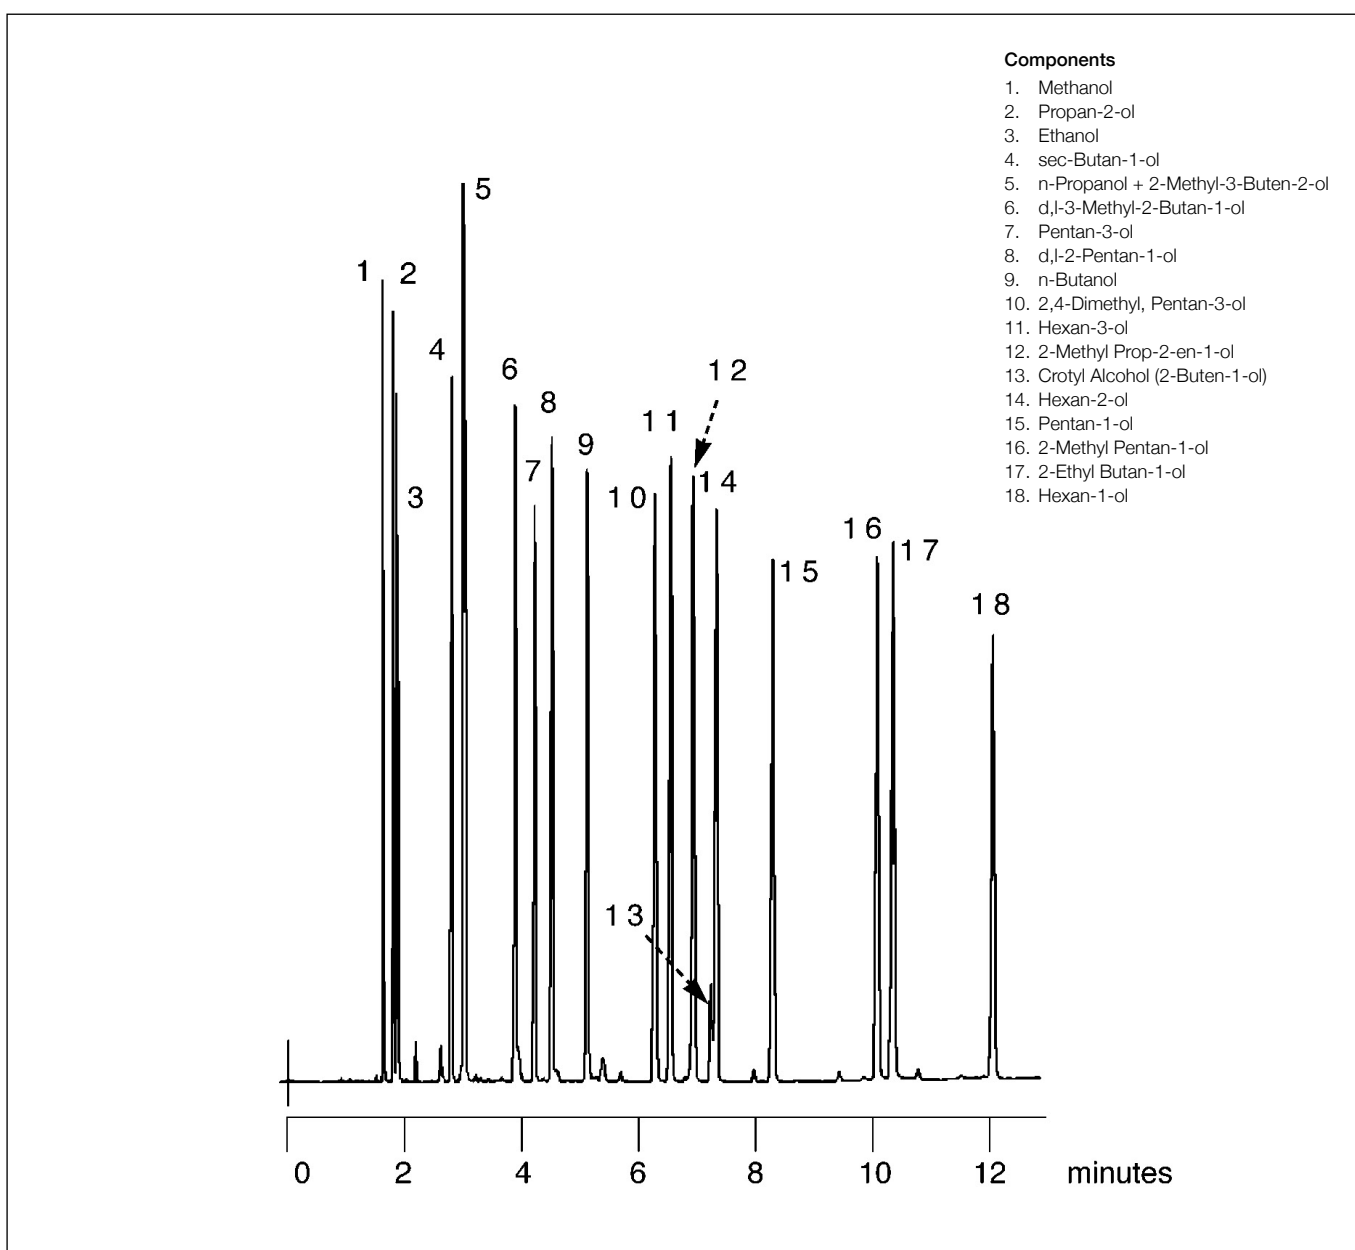


Analysis of 18 alcohols

BP20 (WAX)

Column part number	054427		
Phase	BP20 (WAX)	Final temperature	80°C, 0 min
Column	30 m x 0.25 mm x 0.25 µm	Detector	FID
Initial temperature	45°C, 2 min	Injection mode	Split
Rate	3°C/min	Carrier gas	H ₂


 For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com