

# Moisture Trap (Preconditioned) for Agilent Gas Chromatographs

Part number 5060-9084

## General information

This trap, packed with Molecular Sieve, should be used mainly for removing the trace amount of water that is present in nearly all carrier gases. Trace amounts of water can be detrimental to most liquid phases operated at high temperatures. Many contaminants, other than water, will also be removed by Molecular Sieve 5A.

Fitted with 1/8-inch od Swagelok fittings, the trap is installed directly between the gas line regulator and the gas inlet on the back of the instrument. Since the trap body is constructed of stainless steel, it can be conditioned and regenerated at high temperatures without removing the packing. Its unique S-shape also makes it compact enough to fit in most GC ovens for conditioning and regeneration.

Once in operation, the gas flow pressure drop across the trap is minimal.

## Conditioning

To condition the trap (Figure 1), remove the caps (A) on both ends. Attach one end of the trap to a gas supply with suitable tubing. If the trap has been used, attach the gas supply to the downstream end to reverse the flow direction through the trap.

Since the injection port fitting in some GC ovens is recessed, disconnect the trap and pull it around to the front of the GC. Insert the trap, with the copper tubing still connected to the gas supply, into the oven and close the door securely. Using dry helium or nitrogen, set the flow rate to 60 mL/min and the oven temperature to 350 °C, then condition the trap overnight.

**WARNING:** Remove all columns from the GC oven before conditioning the traps.

If hydrogen is used as purge gas, the exhaust gas should be vented outside the GC oven in a suitable manner.

Reduce the flow to 10 to 30 mL/min and cool the oven. When the oven is cool, disconnect the trap and immediately install it in the desired flow line or seal the trap with the proper tubing plug and cap.

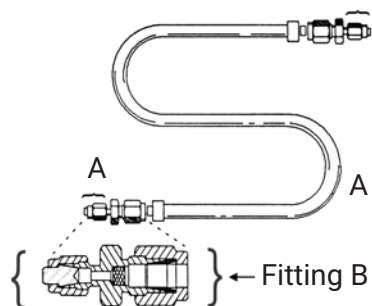


Figure 1. Conditioning the trap.

## Installation

Connect trap in-line between the gas source supply and gas inlet on the instrument, with suitable tubing or adapter fittings.

## Regeneration

Trap regeneration should be done on a periodic basis, i.e., after using one to four cylinders of gas depending on the grade or purity of the gas. The same method and parameters are used for the initial conditioning.

**Table 1.** Ordering information.

Item	Part Number
Conditioned Moisture Trap	5060-9084
Conditioned Hydrocarbon Trap	5060-9096

[www.agilent.com](http://www.agilent.com)

DE24684802

This information is subject to change without notice.

© Agilent Technologies, Inc. 2015, 2022  
Printed in the USA, August 31, 2022

5958-9455

