

# Application News

## No. G292

### Gas Chromatograph

## Analysis of Lower Aliphatic Aldehydes using Nexis GC-2030

Lower aliphatic aldehydes are known to be associated with sick building syndrome. Thus various regulations require strict control of their concentrations. A common method of analyzing lower aliphatic aldehydes is to utilize 2,4-dinitrophenylhydrazine (DNPH) derivatization. Trace level analysis of these compounds is then enabled by using a flame thermionic detector (FTD/NPD).

In this applications news, methods for collecting aldehydes in atmospheric air, extraction and elution using commercially available cartridges and the analysis of lower aliphatic aldehydes using GC-2030 with FTD-2030 are described.

K. Gregory, K. Kawamoto



Fig. 1 Nexis GC-2030

### Sample Collection Method

In this set-up, two commercially available cartridges saturated with 2,4-dinitrohydrazine are connected in series. The pump flow rate is set to about 0.1 L / min, and air sample is collected for 24 hours continuously. The amount of air extraction can be measured by using an integrating flow meter. In order to prevent decomposition of aldehyde-DNPHs by atmospheric ozone, install an ozone scrubber in front of the collection cartridge (Fig. 2).

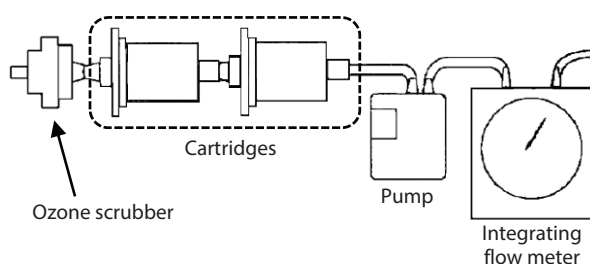


Fig. 2 Schematic Diagram of Collection Method

### Cartridge Elution Method

The aldehydes react in the cartridge to form aldehyde-DNPHs and is eluted with acetonitrile. During elution, unreacted DNPH which may interfere with the analysis may also be eluted. This can be removed by using a cation exchange resin. Since acetonitrile can also be detected by FTD, the eluate should further be extracted with ethyl acetate (Fig. 3).

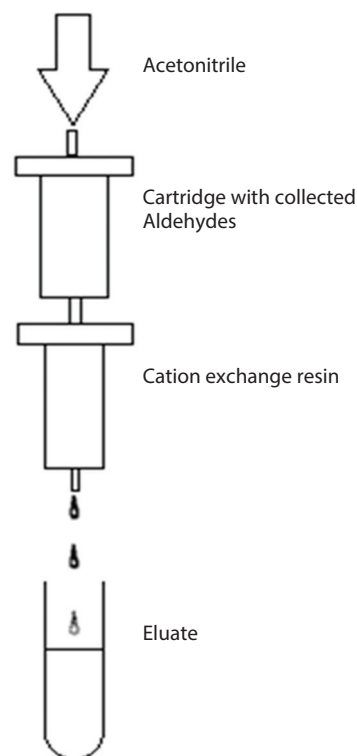
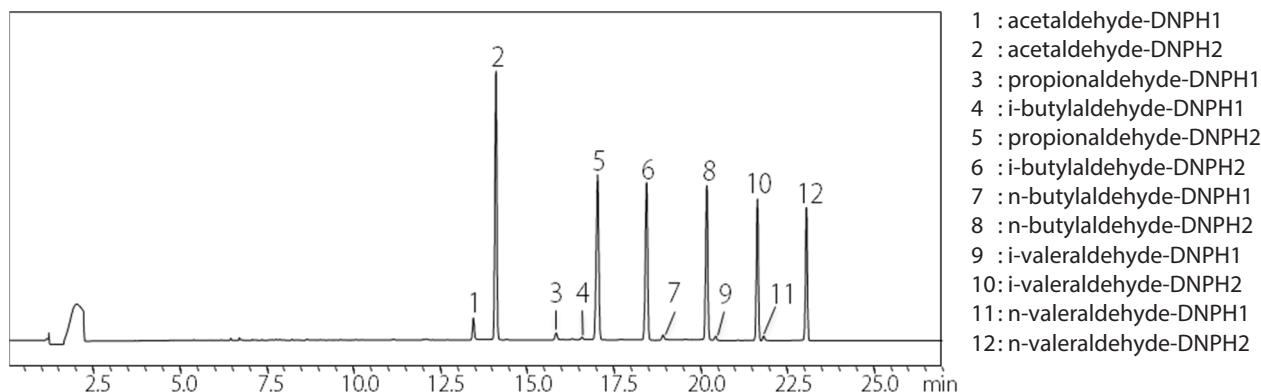


Fig. 3 Schematic Diagram of Elution Method Collection Method

### Note

Trace amounts of aldehydes may also be present in containers, cartridges and in some reagents. Therefore, it is important to always analyze a blank before the actual sample. Depending on the cleanliness of the environment where extraction is performed, it is also possible that unwanted contaminants can make their way to the sample extract.

## ■ Analysis Results



**Fig. 4 Chromatogram for DNPH-Derivatized Lower Aliphatic Aldehydes (1 µg/mL Ethyl Acetate Solution)**

\* Stereoisomers exist for C2 and subsequent aldehydes-DNPH

## ■ Instruments Used and Analytical Conditions

Gas Chromatograph	Nexis GC-2030
Flame Thermionic Detector	FTD-2030
Autosampler	AOC-20i
Software	LabSolutions LC/GC
Injection Unit Temp.	200 °C
Carrier Gas	He (99.999 %)
Carrier Gas Control	Constant linear velocity (41.7 cm/sec, purge flowrate: 3 mL/min)
Injection Mode	Splitless (Sampling time: 1 min; then split (1:30))
Sample Injection Volume	1 mL
Column	Rtx <sup>®</sup> -5 (0.25 mm I.D. × 30 m, d.f. 0.25 mm)
Column Temp.	80 °C (1 min) - 20 °C/min - 200 °C (10 min) - 5 °C/min - 250 °C (0 min) Total 27 min
Detector Temp.	280 °C
Current	1.00 pA
Detector Gas Flowrate	H <sub>2</sub> : 1.5 mL/min, Air: 145 mL/min
Makeup Gas Flowrate	27.5 mL/min (He)

First Edition: Jun. 2017



**For Research Use Only. Not for use in diagnostic procedure.**

This publication may contain references to products that are not available in your country. Please contact us to check the availability of these products in your country.

The content of this publication shall not be reproduced, altered or sold for any commercial purpose without the written approval of Shimadzu. Company names, product/service names and logos used in this publication are trademarks and trade names of Shimadzu Corporation or its affiliates, whether or not they are used with trademark symbol "TM" or "®". Third-party trademarks and trade names may be used in this publication to refer to either the entities or their products/services. Shimadzu disclaims any proprietary interest in trademarks and trade names other than its own.

The information contained herein is provided to you "as is" without warranty of any kind including without limitation warranties as to its accuracy or completeness. Shimadzu does not assume any responsibility or liability for any damage, whether direct or indirect, relating to the use of this publication. This publication is based upon the information available to Shimadzu on or before the date of publication, and subject to change without notice.

Shimadzu Corporation

[www.shimadzu.com/an/](http://www.shimadzu.com/an/)