


Analysis of amines

BPX5

Column part number	054113		
Phase	BPX5	Final temperature	360°C
Column	25 m x 0.22 mm x 0.25 µm	Detector	FID, 380°C
Initial temperature	40°C, 1 min	Injector	Split
Rate	8°C/min	Carrier gas	H ₂ , 12 psi

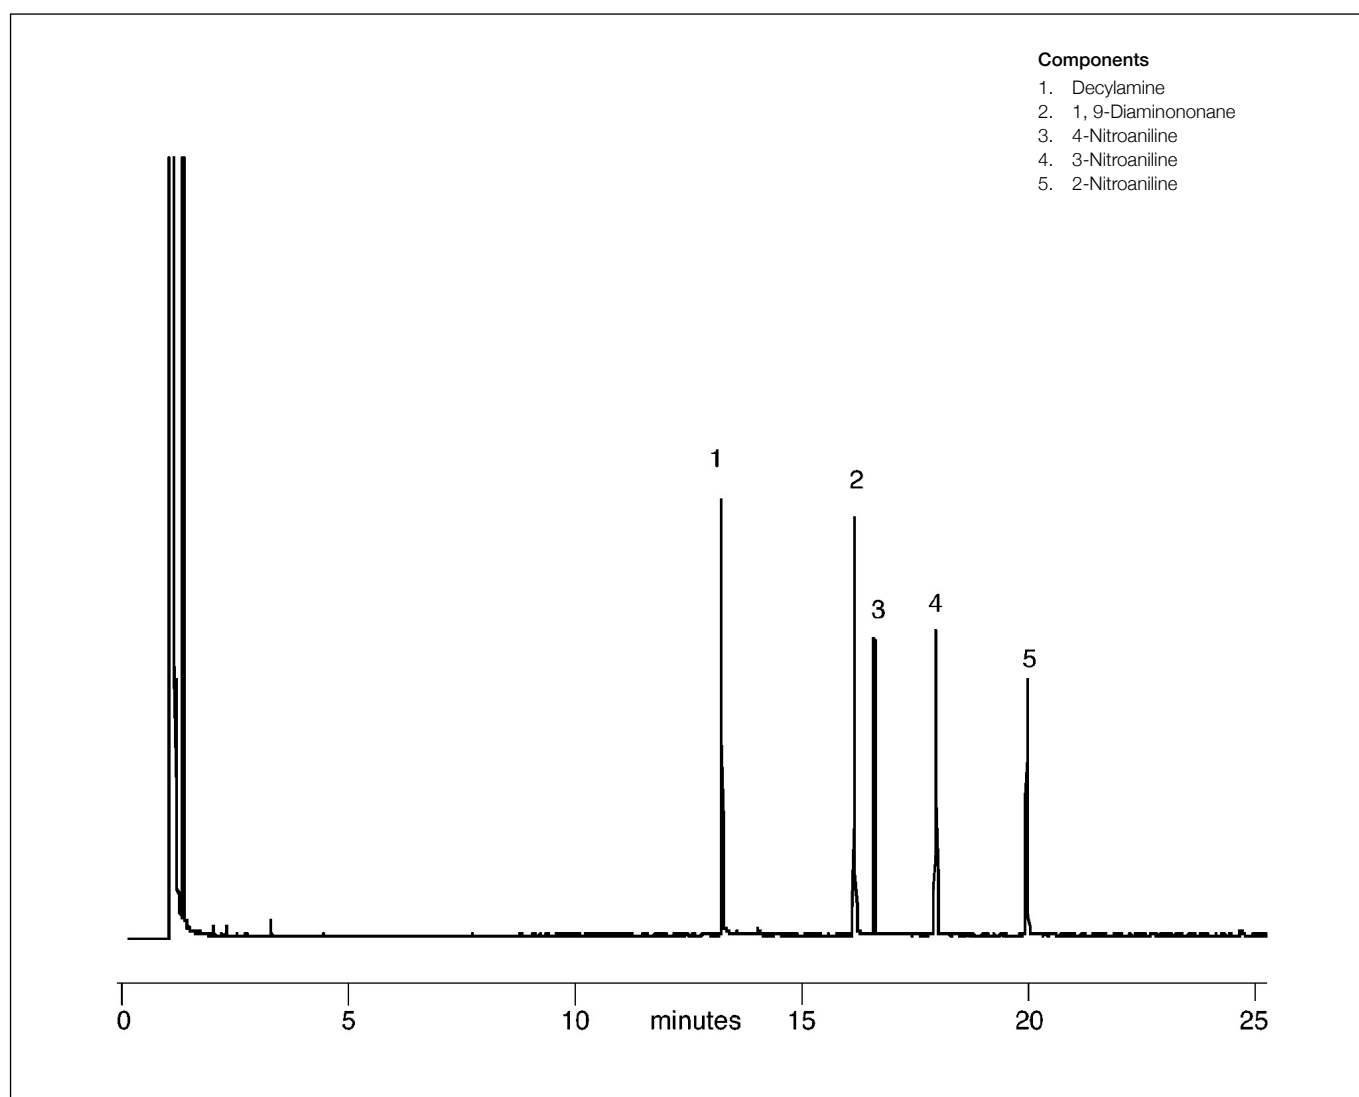

For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com