

Method Modernization for Routine Analysis of Biotherapeutics as Part of Lifecycle Management

Ximo Zhang, Robert Birdsall, and Ying Qing Yu
Waters Corporation, Milford, MA, USA

APPLICATION BENEFITS

- Method modernization using ACQUITY® UPLC® H-Class Bio System for improved productivity and reduced method complexity in the routine analysis of small biotherapeutics.
- Increased throughput for identity testing of small biotherapeutics.
- Robust and specific platform method that can be applied to various biotherapeutic analogues.

WATERS SOLUTIONS

[ACQUITY UPLC H-Class Bio System](#)

[ACQUITY UPLC Tunable Ultra-Violet \(TUV\) Detector](#)

[ACQUITY UPLC Peptide CSH™ Column](#)

[Empower® 3 Software](#)

KEYWORDS

Insulin, biotherapeutics, monograph, lifecycle management

INTRODUCTION

The fast growing market of biotherapeutics brings certain challenges for pharmaceutical development and quality control, such as throughput, robustness, and cost. This in part is due to using the United States Pharmacopeia USP monographs that were developed using dated instruments and methods. While USP monographs offer the distinct advantage of not requiring re-validation when deployed in the routine analysis of biotherapeutics, these analyses often require excessive resources, such as long analysis time and large solvent consumption. As of 2011, the USP has embarked on an initiative to modernize more than 2000 monographs, including both physiochemical tests and bioassays, deviation from which will require justification on the manufacturer's part. As part of a sound pharmaceutical system, the International Committee on Harmonization (ICH) recommends continual improvement, including the evaluation of new and innovative technologies and methods to ensure product quality and safety.¹ To this end, method modernization affords pharmaceutical companies the ability to address challenges associated with manufacturing for rapidly growing markets with efficient workflows that are aligned with regulatory guidelines while maintaining product quality and safety.

The objective of this work is to demonstrate how the modernization of a USP monograph can increase throughput and productivity in a routine environment. In this study, insulin is selected as an example for its historical precedence and significant market size.² A new method for identity test will be developed and performed on three insulin analogues to compare with the methods in supporting monographs.

EXPERIMENTAL

Chemical and reagents

Insulin human, insulin lispro, and insulin glargine were purchased from USP. Endoproteinase Glu-C from *S. aureus* was purchased from Promega. Digestion and separation procedures were as outlined in the *USP monograph: insulin human*,³ *insulin lispro*,⁴ and *insulin glargine*.⁵ New separation methods were also developed as shown in the gradient table. HPLC grade water, acetonitrile, and TFA were purchased from Fisher Scientific and used as received.

LC conditions

USP method and scaled USP method

LC system:	Alliance® HPLC
Detectors:	e2489 UV detector, 5 mm flow cell, $\lambda = 215$ nm
LC column:	XSelect® CSH C ₁₈ Column 3.5 μ m, 130 Å, 4.6 mm x 100 mm (P/N 186005269)
Column temp.:	40 °C for insulin human and lispro 35 °C for insulin glargine
Sample vial:	12 x 32 mm glass vial, total recovery (P/N 600000750cv)
Mobile phase:	Water and acetonitrile
MP additive:	Sulfate buffer for insulin human and lispro, phosphate buffer for insulin glargine
Mass load:	8.6 μ g

Gradient table for geometrically scaled USP method

Time (min)	Flow rate (min)	%A	%B
Initial	0.428	90.0	10.0
29.14	0.428	30.0	70.0
31.57	0.428	0.0	100.0
34.00	0.428	0.0	100.0
34.49	0.428	90.0	10.0
41.77	0.428	90.0	10.0

Gradient table for developed method

Time (min)	Flow rate (min)	%A	%B
Initial	0.300	85.0	15.0
10.00	0.300	55.0	45.0
11.00	0.300	0.0	100.0
13.00	0.300	0.0	100.0
13.50	0.300	85.0	15.0
20.00	0.300	85.0	15.0

Developed method

LC system:	ACQUITY UPLC H-Class Bio
Detectors:	ACQUITY TUV Detector, 5 mm flow cell, $\lambda = 215$ nm
LC column:	ACQUITY UPLC CSH C ₁₈ 1.7 μ m, 130 Å, 2.1 mm x 100 mm (P/N 186006937)
Column temp.:	40 °C
Sample vial:	12 x 32 mm glass vial, total recovery (P/N 600000750cv)
Mobile phases:	Water and acetonitrile
MP additive:	0.1% TFA
Mass load:	0.86 μ g

RESULTS AND DISCUSSION

Insulin human is a 5.8 kDa protein that consists of two polypeptide chains (Figure 1). Since its first clinical application in 1922, insulin drugs have undergone rapid development with six analogues now available on the market for different drug activities.⁶ These analogues have highly similar structures with only slight amino acids difference in sequence. Supporting USP monographs for identity test of each of these analogues also vary from one another with changes in mobile phase, gradient, flow rate, and temperature.^{3,4,5} To establish a baseline for modernization, the identity tests for these insulin analogues (insulin human, insulin lispro, and insulin glargine) were performed using methods as outlined in their respective USP monograph. An XBridge[®] CSH C₁₈ Column with L1 packing was selected for better peak shape in HPLC separation. Proteolytic cleavage of each analogue produced four peptide fragments that were well resolved using the HPLC method described in each monograph (Figure 2). While sufficient in their current format, it should be noted that the long run times (86 min for insulin human) associated with HPLC can be reduced by updating to a UPLC-based method for improved throughput and reduced waste stream.

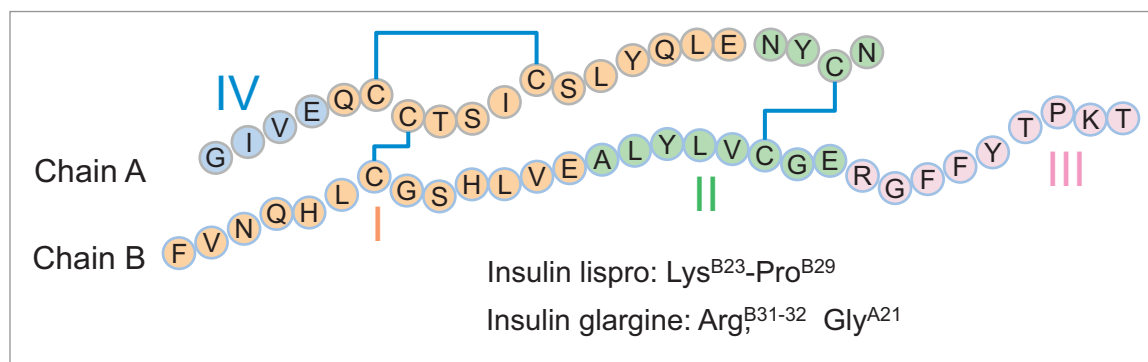


Figure 1. Structure of insulin human. Insulin lispro and insulin glargine have slightly different amino acid sequences. Peptide fragments generated via Glu-C digestion are color-coded and labeled from I to IV.

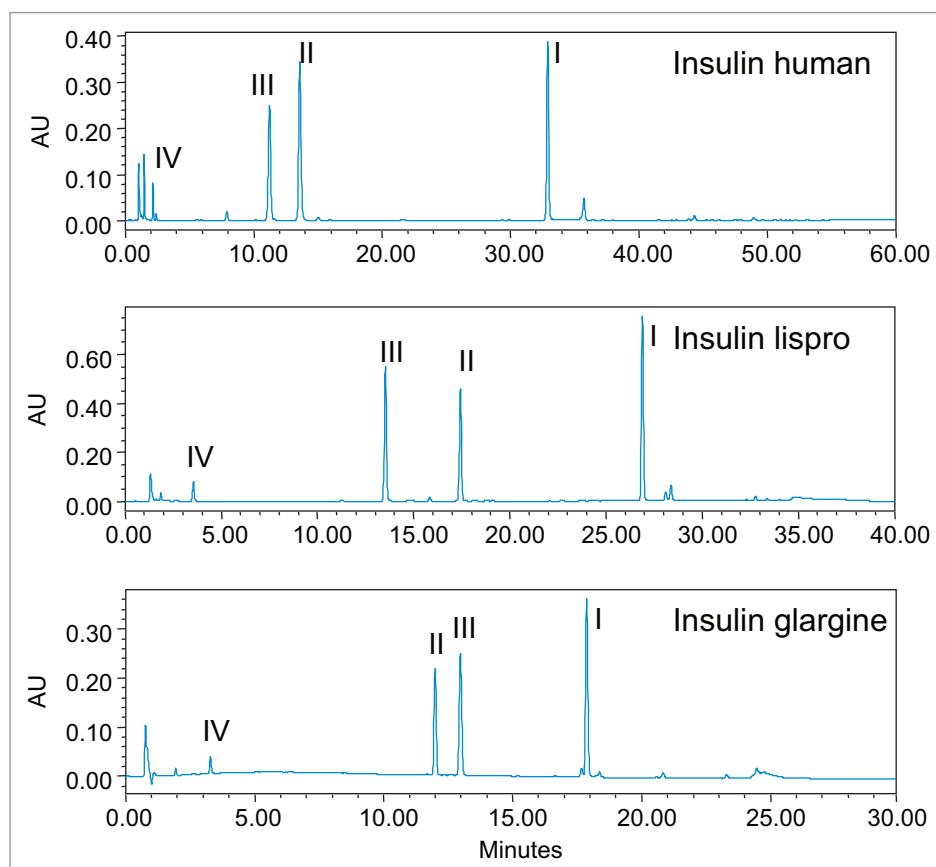


Figure 2. Identity test of insulin human, insulin lispro, and insulin glargine following the procedures in USP monographs. The four peptide fragments were well separated under each condition. Sulfate buffer was used as mobile phase additive for insulin human and insulin lispro while phosphate buffer was used for insulin glargine. Other experimental conditions were described in Experimental Section.

To demonstrate the benefit of a UPLC-based method, USP Chapter <621>⁷ was referenced for acceptable method changes. As described in <621>, a column with 50% smaller particle size was used along with geometrically scaled gradient conditions to reduce the analysis time. An ACQUITY UPLC H-Class Bio System was used to accommodate the higher pressure generated by columns packed with smaller particles. With a 1.7 μm particle size column, the analysis time was reduced from 60 min (Figure 3A) to 30 min (Figure 3B) for insulin human using the scaled method for improved productivity. It should be noted that the monograph results shown in Figure 2 use different buffer additives which may not be ideal for streamlining the manufacturing process, specifically in the case of a manufacturer with multiple insulin analogues in their product pipeline. To address this challenge we need to consider method development changes beyond USP <621> limitations. With this in mind, TFA was used as a mobile phase additive for the identity test of insulin human. With a 10 min gradient from 15% to 45% mobile phase B, separation time was reduced by 75% from the original USP method as shown in Figure 3C. The impact of TFA on selectivity and resolution was evaluated as shown in Table 1. Comparable selectivity and baseline resolution were observed for the majority of the peptide fragment peaks using the new high-throughput method when compared to the monograph-based methods, suggesting the method could be utilized as a 'platform' assay for various insulin analogues.

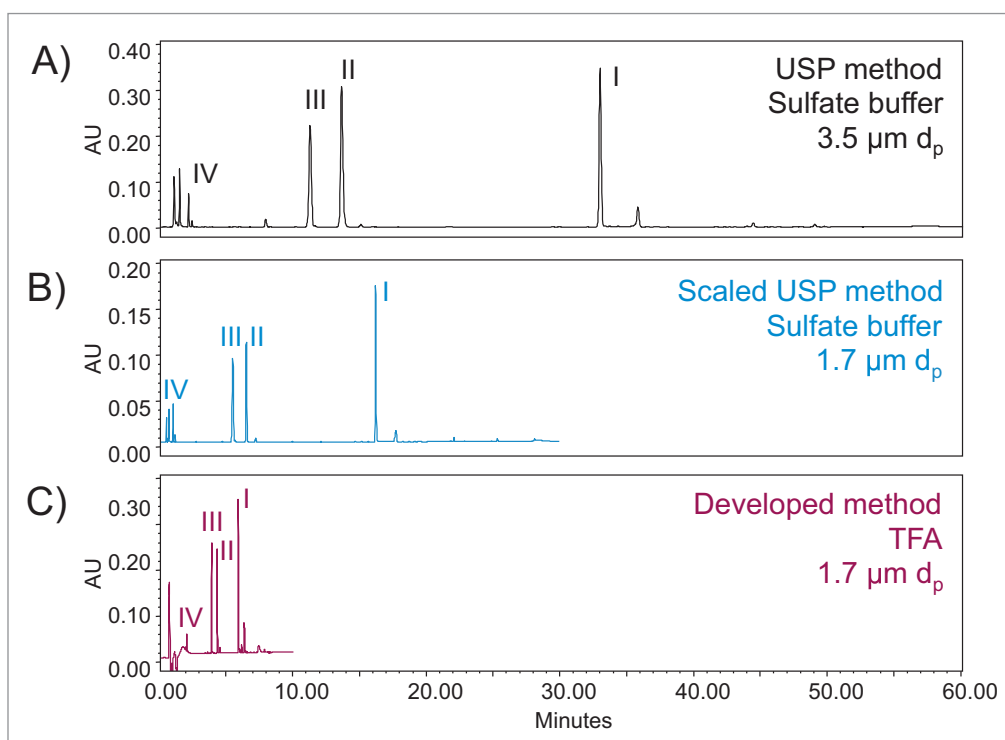


Figure 3. Comparison of identity test of insulin human using the USP monograph method (3A), scaled USP method (3B), and the method developed beyond USP 621 limit (3C). Above chromatograms show the key stage of separation. A column with 1.7 μm particle size was used in scaled USP method, which enabled the use of a shorter gradient time. With TFA as mobile phase additive, the gradient time was further reduced to 10 minutes.

Table 1. Comparison of selectivity and resolution on USP method, scaled USP method, and beyond USP method. The developed method showed comparable selectivity and resolution with USP method while reducing the analysis time by 75%.

	Selectivity			Resolution		
	IV-III	IV-II	IV-I	IV-III	III-II	II-I
USP method	9.3	1.2	2.7	38.5	8.1	68.0
Scaled USP method	10.1	1.2	2.6	44.8	7.6	91.2
Developed method	3.2	1.2	1.5	40.5	7.2	34.1

With the same method condition, the developed method was applied on insulin lispro and insulin glargine. As shown in Figure 4, the peptide fragments were well resolved for all three insulin analogues in an 8 min elution window. The top five most abundant peaks were identified as fragment I-IV, and a pyroglutamic form of fragment I. The same retention time was observed for peptide fragment IV and I across samples due to their identical structures. The retention time of peptide fragment III in insulin lispro and II, III in insulin glargine shifted from the peptide fragments peaks found in insulin human due to minor differences in their primary sequence (Figure 1), suggesting the method is robust and specific to various insulin analogues. Collectively, this study demonstrates 'finger-print'-like analyses can be developed as efficient and robust platform methods used in routine analysis of insulin analogues.

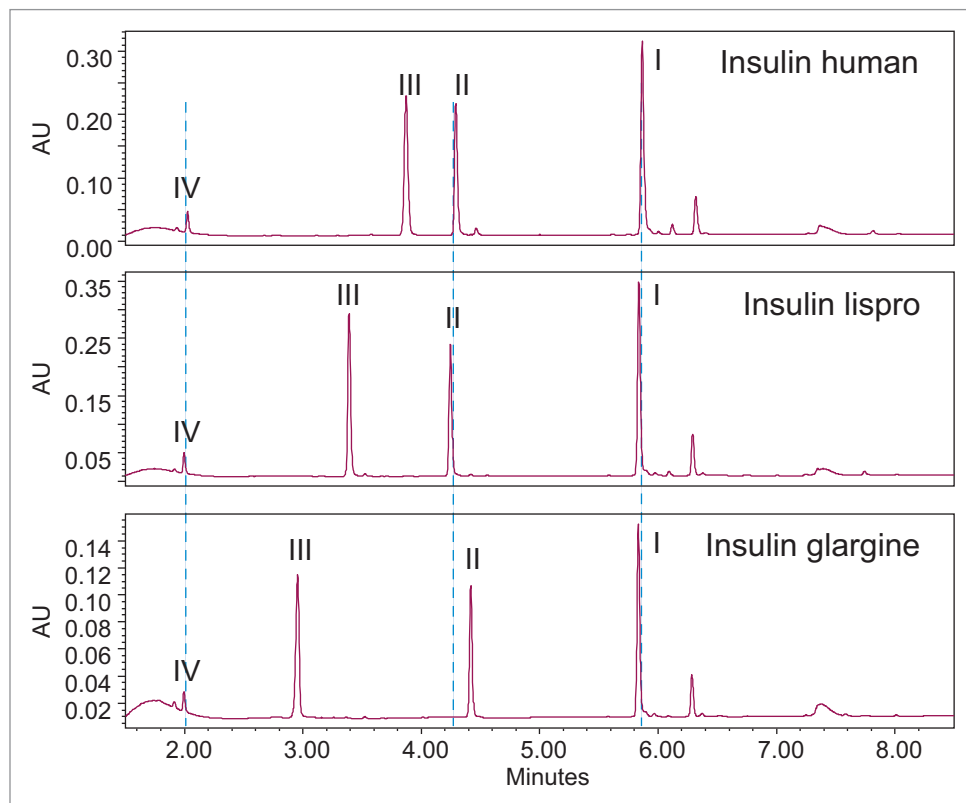


Figure 4. Identity test of insulin analogues using the developed method with 1.7 μ m particle size column and TFA as mobile phase additive. Good resolution was obtained across all peaks. In addition, peptide fragments with identical amino acid are aligned with the same retention time making it an ideal platform method that can be efficiently deployed for routine analysis of insulin analogues.

CONCLUSIONS

This work demonstrated the modernization of the USP monograph for high-throughput identity test of insulin analogues. Using a sub-2- μm particle size column and ion-pairing reagent TFA, the HPLC-based USP method was updated to an UPLC-based method with higher efficiency for the separation of digested peptides of insulin analogues. Compared to original USP methods, the developed method reduced analysis time by 75% with comparable resolution and can be applied to multiple insulin analogues, making it an ideal platform method for insulin analysis in a routine environment.

References

1. Guidance for industry Q10 pharmaceutical quality system. ICH, 2009.
2. Human insulin market. *Zion Market Research*. 2016.
3. USP monograph: insulin human [11061-68-0]. 2015, Revision Bulletin.
4. USP monograph: insulin lispro. USP 39-NF 34, 2015, Revision Bulletin.
5. USP monograph: insulin glargine [160337-95-1]. 2016, Revision Bulletin.
6. Hsu, J., et al. Identification of recombinant insulin analogues by peptide mapping method. *Journal of Food and Drug Analysis*. 2012, 20, 4:957-962.
7. <621> Chromatography, US Pharmacopeia, USP 38-NF33 S1.

Waters

THE SCIENCE OF WHAT'S POSSIBLE.®

Waters, The Science of What's Possible, ACQUITY, UPLC, Alliance, XSelect, XBridge, and Empower are registered trademarks of Waters Corporation. CSH is a registered trademark of Waters Corporation. All other trademarks are the property of their respective owners.

Waters Corporation
34 Maple Street
Milford, MA 01757 U.S.A.
T: 1 508 478 2000
F: 1 508 872 1990
www.waters.com