


Analysis of aniline impurities

BPX5

Column part number	054127		
Phase	BPX5	Rate 2	20°C/min
Column	12 m x 0.32 mm x 1.0 µm	Final temperature 2	330°C, 10 min
Initial temperature	50°C, 1 min	Detector	FID, 380°C
Rate 1	15°C/min	Injector	Split
Final temperature 1	120°C	Carrier gas	He, 4 psi

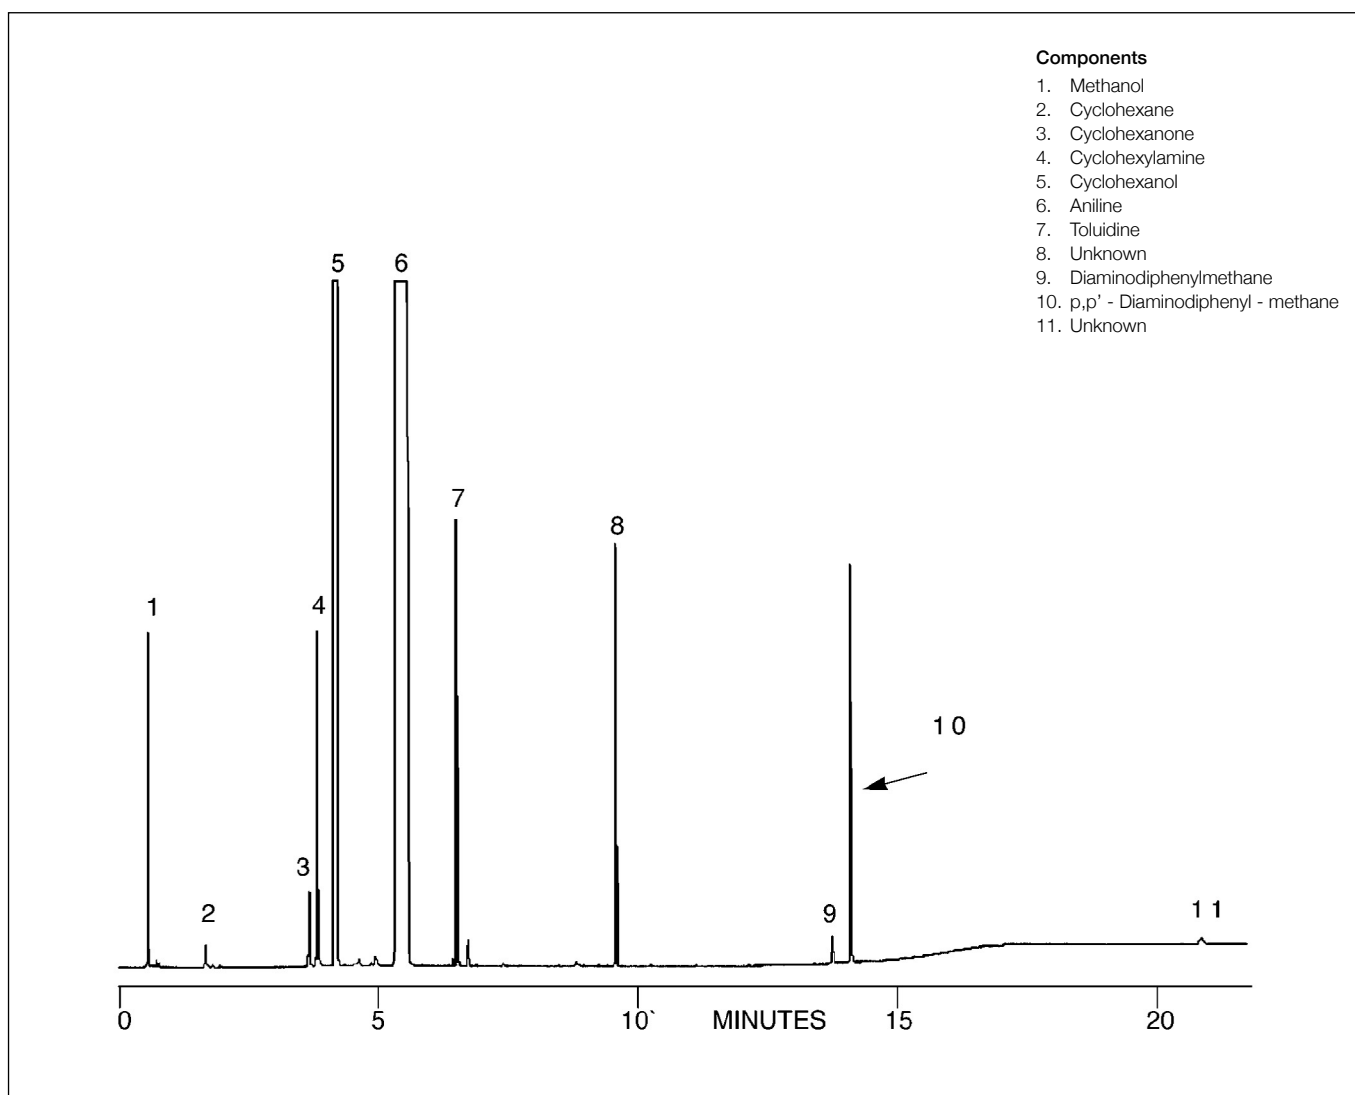

For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com