



Nitro compounds

Application Note

Environmental

Authors

Agilent Technologies, Inc.

Introduction

Analysis of eight nitro compounds by gas chromatography using an Agilent FactorFour VF-1301ms column in less than 25 minutes.



Agilent Technologies


Conditions

Technique : GC-capillary
Column : Agilent FactorFour VF-1301ms, 0.25 mm x 30 m
fused silica (df = 0.25 μ m) (Part no. CP9053)
Temperature : 45 °C (3 min) \rightarrow 280 °C, 10 °C/min
Carrier Gas : He, 60 kPa
Injector : Split, 1 μ L, 1:100
Detector : FID
Sample : 2000 μ g/ μ L in methanol

Courtesy : J. Peene, Agilent application laboratory,
Middelburg, The Netherlands

Peak identification

1. aniline
2. benzyl alcohol
3. 4-chloroaniline
4. 2-methylnaphthalene
5. 2-nitroaniline
6. 3-nitroaniline
7. dibenzofuran
8. 4-nitroaniline

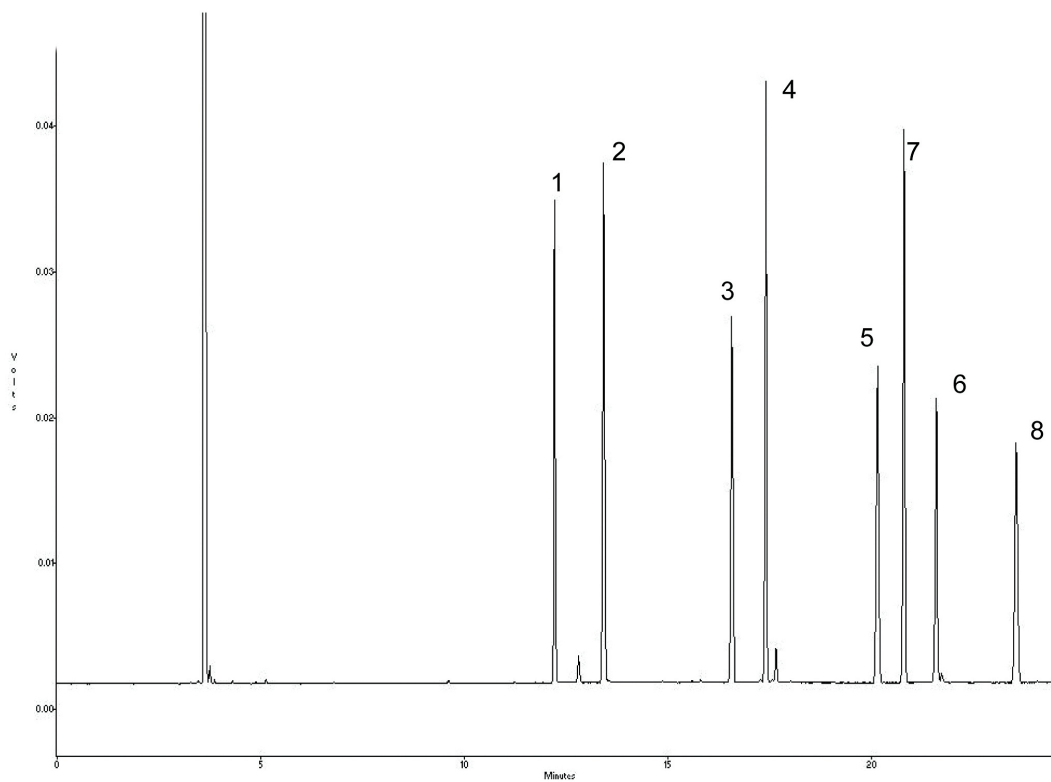

www.agilent.com/chem

This information is subject to change without notice.

© Agilent Technologies, Inc. 2011

Printed in the USA

31 October, 2011

First published prior to 11 May, 2010

A02415



Agilent Technologies