



Gases

Fast analysis of inert gases

Application Note

Environmental

Authors

Agilent Technologies, Inc.

Introduction

Fast GC analysis of inert gases in less than 150 seconds is achieved using an Agilent PorapLOT Q column and Agilent 490 Micro GC.



Agilent Technologies


Conditions

Technique : Micro-GC
Column : Agilent PoraPLOT Q, 0.32 mm x 10 m fused silica
PLOT (df = 10 μ m)
Temperature : 30 °C
Carrier Gas : He, 50 kPa (0.5 bar, 7 psi)
Heated Injector : no
Injection Time. : 30 msec
Concentration Range : high
Matrix : oxygen

Courtesy : Pascal Vattaire/Jean-Luc Barranca,
Agilent France S.A.

Peak identification

1. methane
2. krypton
3. carbon dioxide (CO₂)
4. nitrous oxide (N₂O)
5. xenon

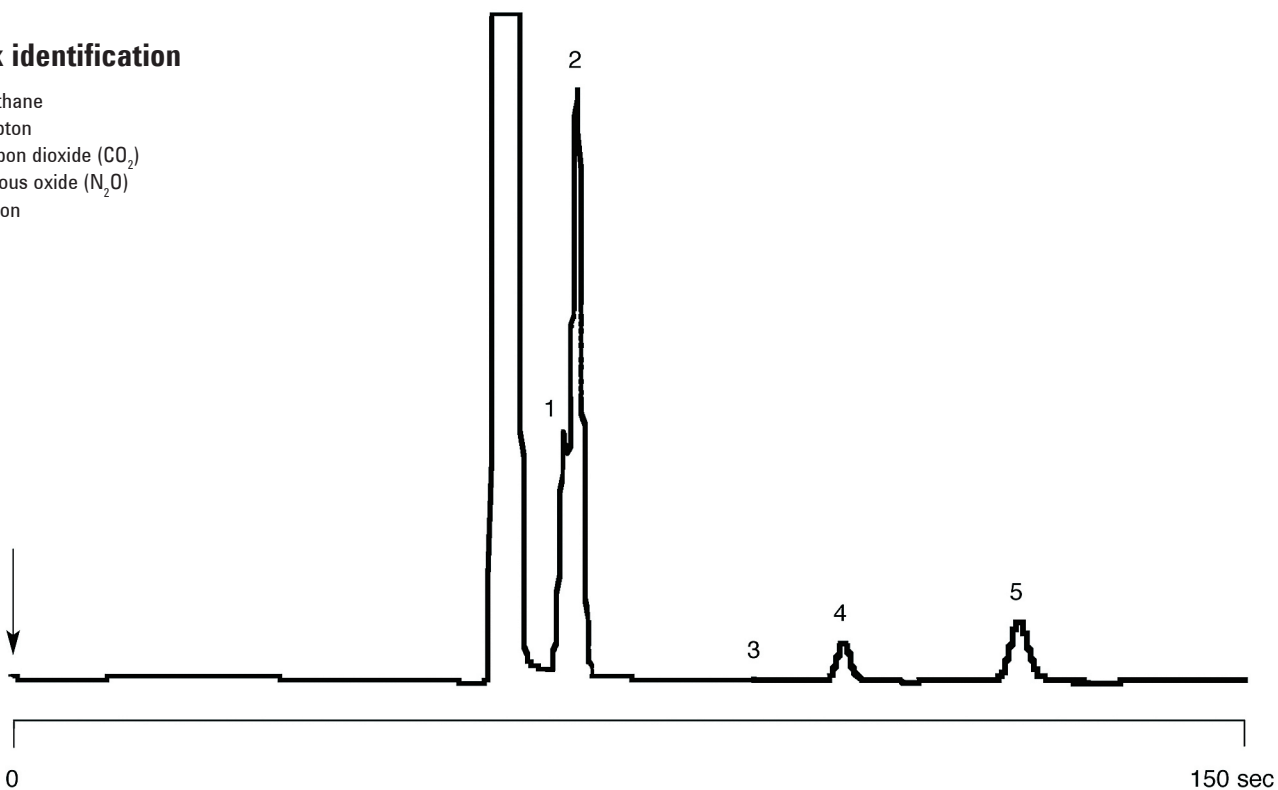

www.agilent.com/chem

This information is subject to change without notice.

© Agilent Technologies, Inc. 2011

Printed in the USA

31 October, 2011

First published prior to 11 May, 2010

A01633



Agilent Technologies