



Pyrolysis products of a sample containing oils

Application Note

Materials Testing & Research

Authors

Agilent Technologies, Inc.

Introduction


Analysis of a pyrolysis sample containing two oil fractions is accomplished by GC with an Agilent VF-5ms column.



Agilent Technologies

Conditions

Technique : GC
Column : Agilent VF-5ms, 0.25 mm x 60 m fused silica
(df = 1.0 μ m) (Part No. CP8949)
Temperature : 60 °C, 1 min \rightarrow 320 °C, 8 °C/min, 75 min
Carrier Gas : He, 173 kPa
Pyrolysis : at 550 °C
Injector : Split injection, 1:100
Detector : MS

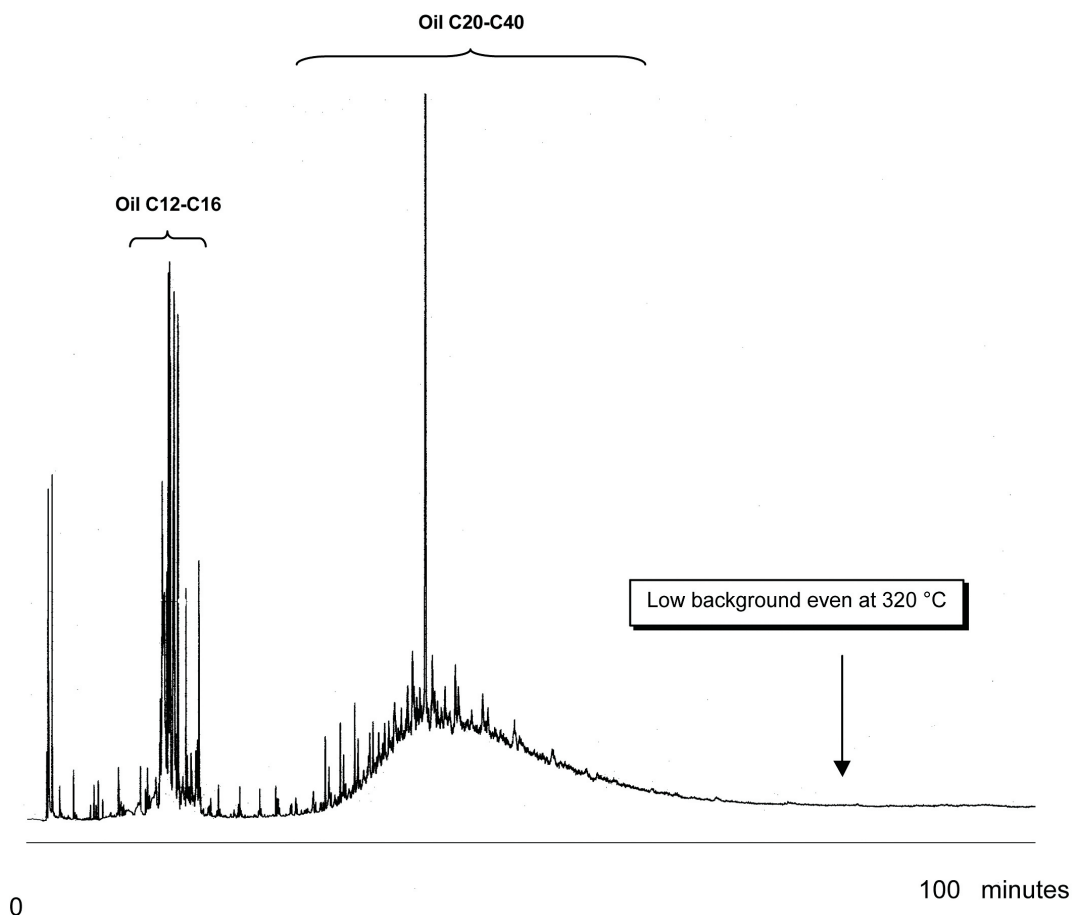

www.agilent.com/chem

This information is subject to change without notice.

© Agilent Technologies, Inc. 2011

Printed in the USA

31 October, 2011

First published prior to 11 May, 2010

A02260



Agilent Technologies