
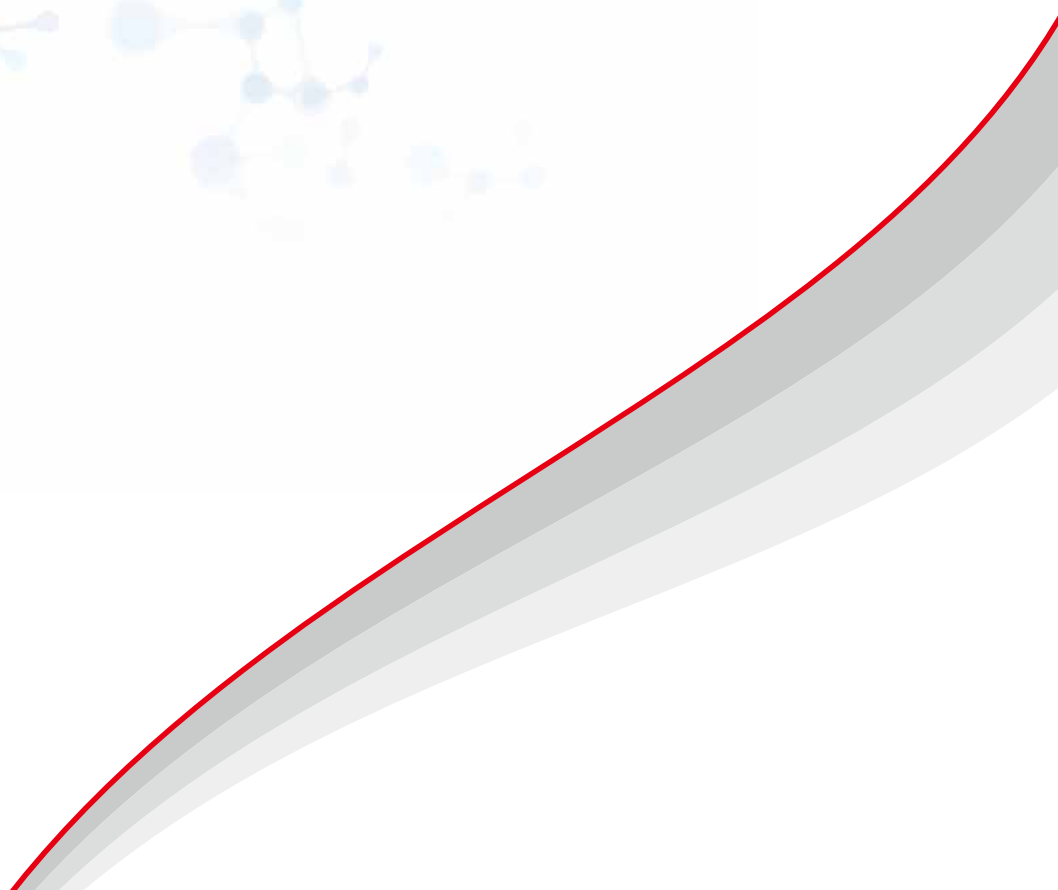


Maximize LC Separation Performance with Core Shell Technology

Shim-pack Velox LC Columns

CoreFocus




Maximize LC Separation Performance with Core Shell Technology

Designed to maximize performance of LC systems, Shimadzu's Shim-pack™ Velox columns with core shell technology enable you to achieve increased separations and faster analysis times on any LC platform.

Whether developing a high efficiency LC separation method, transferring an existing method for increased throughput while maintaining resolution, or are trying to improve the resolution of a complex separation, Shim-pack Velox™ columns will satisfy your needs.

Column ruggedness is critical to any LC analysis and Shim-pack Velox core-shell columns deliver excellent column lifetime for even the most challenging sample matrices.



Shim-pack Velox column will deliver

- Increased resolution with maximum efficiency → improving separation and detection
- Faster separation without sacrificing performance → maximizing laboratory productivity and reducing cost of analysis
- Increased sample throughput → reducing overall analysis time
- Superior ruggedness → reducing cost of analysis
- Excellent reproducibility → maintaining analysis and data integrity

Column Selection Guide for Different LC Platforms

Column particle sizes and column volumes affect chromatography results significantly if the column configuration does not match the LC system. As column particle size is reduced, or the column volume (ID and/or the length of the columns) decreases, the necessity for a lower dispersion system is increased.

Choosing the optimal column configuration for your LC system allows you to achieve improved chromatography. The following table summarizes the starting recommendations of column configuration for each LC system.



Nexera

Ultra High Performance Liquid Chromatograph




i-Series

High Performance Liquid Chromatograph

	Nexera lite LC-2050	Nexera XR LC-2060	Nexera XS Nexera X3
LC System	HPLC	UHPLC-like	UHPLC
Particle size	2.7 μm & 5 μm	2.7 μm	1.8 μm & 2.7 μm
Column I.D.	4.6 mm (3.0 mm)	3.0 mm (2.1 mm)	2.1 mm
Column Length	100-250 mm	50-100 mm	≤150 mm

Column Chemistries

Combining highly efficient core shell particle technology with a wide range of surface chemistries provides you with the best opportunity for optimal resolution. With different chemistry characteristics, Shim-pack Velox columns are suitable for use in a wide variety of applications and challenging separations.

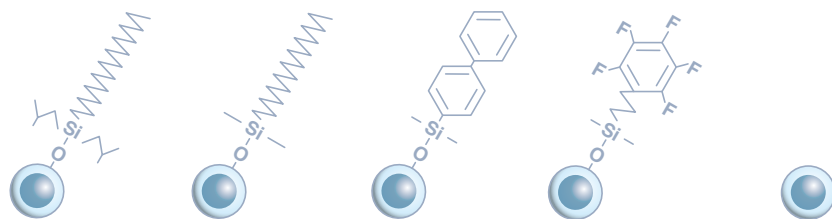


		SP-C18	C18	Biphenyl	PFPP	HILIC
USP Classification		L1	L1	L11	L43	L3
Ligand type		Sterically protected C18	C18	Biphenyl	Pentafluorophenyl propyl	None
Particle Size (µm)		1.8, 2.7, 5	1.8, 2.7, 5	1.8, 2.7, 5	1.8, 2.7, 5	2.7
Pore size (Å)		90	90	90	90	90
Surface Area	1.8 µm	125 m ² /g	125 m ² /g	125 m ² /g	125 m ² /g	130 m ² /g
	2.7 µm	130 m ² /g	130 m ² /g	130 m ² /g	130 m ² /g	
	5 µm	100 m ² /g	100 m ² /g	100 m ² /g	100 m ² /g	
Carbon Load	1.8 µm	7 %	9 %	7 %	4 %	N/A
	2.7 µm	7 %	7 %	7 %	4 %	
	5 µm	5 %	5 %	5 %	3 %	
End-Cap		No	YES	YES	No	No
pH range		1.0-8.0	2.0-8.0	1.5-8.0	2.0-8.0	2.0-8.0
Max Pressure	1.8 µm	100 MPa*	100 MPa*	100 MPa*	100 MPa*	60 MPa
	2.7 µm	60 MPa	60 MPa	60 MPa	60 MPa	
	5 µm	40 MPa	40 MPa	40 MPa	40 MPa	

* For maximum lifetime, recommended maximum pressure for 1.8 µm particles is 80MPa.

Lot to Lot Reproducibility

We understand that lot to lot consistent performance of columns is required to maximize your laboratory performance. From one lot to the next, every Shim-pack Velox column you purchase will perform consistently.

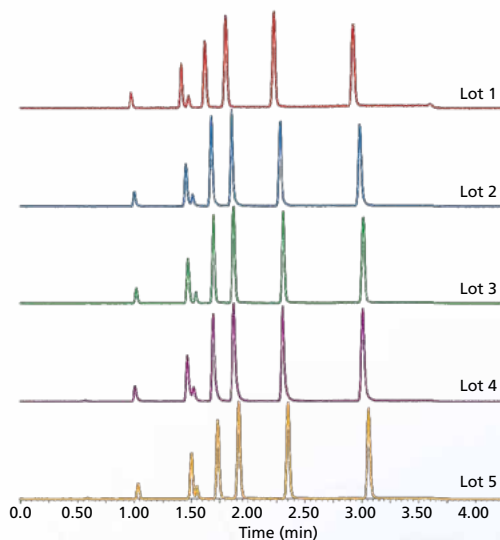

Compounds (50 ng/mL) :

1. Cortisol
2. 11-Deoxycortisol
3. Estradiol
4. Boldenone
5. Testosterone
6. Androstenedione
7. Progesterone

Column: Shim-pack Velox Biphenyl 2.7 µm, 3.0×100 mm
(P/N: 227-32016-03)

Flow Rate: 0.7 mL/min

Column Temp.: 30 °C

Sample Diluent: Initial mobile phase

Injection Volume: 5 µL

Mobile Phase A: 0.1 % formic acid in water

Mobile Phase B: 0.1 % formic acid in acetonitrile

Gradient: 40 % B (0 min) → 80 % B (3 min)

→ 40 % B (3.01 min – 5 min)

Shim-pack Velox SP-C18




Designed and intended specifically for use under low pH condition, Shim-pack Velox SP (Sterically Protected)-C18 offers a well balanced retention profile with a long life time even under harsh, acidic condition needed for LC/MS(/MS) analysis.

- Sterically protected to resist strongly acidic (pH 1-3) mobile phase condition
- Well balanced retention profile
- Suitable for LC/MS(/MS) analysis


Low pH Stability

Sterically protected ligand provides extended low pH stability for the core shell particle. Shim-pack Velox SP-C18 columns maintain a stable retention profile under strongly acidic mobile phase condition (pH1) .

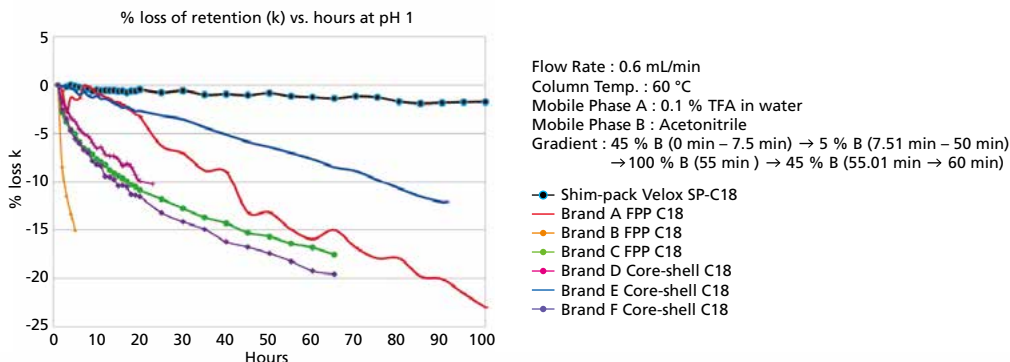

Simultaneous Analysis of 22 Preservative Agents

More than 20 compounds used as the preservative agent for industrial products like foods and cosmetics can be separated by Shim-pack Velox SP-C18. The simultaneous determination and quantitation of multiple target compounds are possible in a wide range of commercial product within acceptable analytical times.

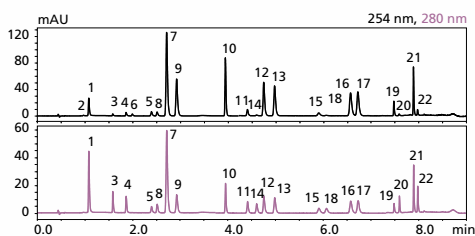


Preservative agents

- | | |
|-----------------------------------|-------------------------------|
| 1 2-methyl-4-Isothiazolin-3-one | 12 Isopropyl Paraben |
| 2 2-Bromo-2-Nitro-1,3-propanediol | 13 Propyl Paraben |
| 3 Salicylic Acid | 14 4-Chloro-3-Methylphenol |
| 4 Isothiazolinones | 15 Ethyl Benzoate |
| 5 Benzoic Acid | 16 Isobutyl 4-Hydroxybenzoate |
| 6 Benzyl Alcohol | 17 Butyl Paraben |
| 7 Sorbic Acid | 18 Chloroxylenol |
| 8 2-Phenoxyethanol | 19 Phenyl Benzoate |
| 9 Methyl Paraben | 20 Clorofene |
| 10 Ethyl Paraben | 21 Triclocarban |
| 11 Methyl Benzoate | 22 Triclosan |

LC Conditions

Column: Shim-pack Velox SP-C18, 2.7 μm, 3.0x100 mm (PN: 227-32004-03)
 Flow Rate: 1.0 mL/min
 Column Temp.: 45 °C
 Mobile Phase A: NaH₂PO₄ aq. (25 mM, pH3.8)
 Mobile Phase B: MeOH/ACN = 9/1
 Gradient: 8 % B (0 min) → 30 % B (0.7 min – 2.7 min) →
 47 % B (2.71 min – 5min) → 52 % B (6 min) →
 80 % B (7 min – 8 min) → 8 % B (9.01 min -10 min)
 Injection Volume: 1 μL
 Conc.: 50 mg/L

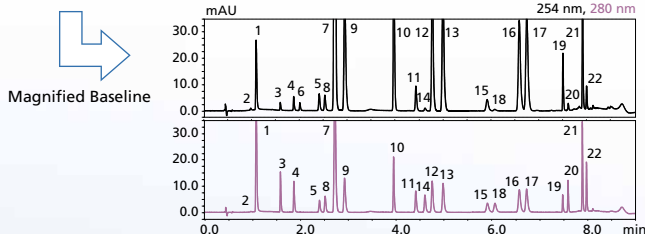

Shim-pack Velox C18



Shim-pack Velox C18 is a traditional end-capped C18-bonded phase which offers the highest hydrophobic retention of any Shim-pack Velox phases and is applicable to a wide range of applications such as pharmaceutical, food, environmental and clinical and neutrals at moderately low and mid-range pH.

- General purpose column for reversed-phase chromatography
- Highest hydrophobic retention among Shim-pack Velox series
- Compatible with moderately acidic to neutral mobile phases (pH 2-8)

Method Transfer for Cyanocobalamin Analysis within the USP Allowable Adjustment

The assay of cyanocobalamin (a synthetic form of vitamin B12) with 5 µm fully-porous ODS column described in the USP monograph is transferred to a new method with Shim-pack Velox C18 2.7 µm column, within USP allowable adjustments. Analytical time and solvent consumption can be saved with transferred methods while meeting the requirements of system suitability.

USP requirement of Chromatography <621>

When the column size is changed, the following conditions should be met;

1) L/dp ratio: within -25 % to +50 %


or

Number of theoretical plates (N): within -25 % to +50 % (For SPP)

2) Flow rate: *Based on particle size and internal diameter and ±50%


$$* F_2 = F_1 \times \frac{dc_2^2 \times dp_1}{dc_1^2 \times dp_2}$$

L : Column length
 dp : Particle size
 F : Flow rate
 dc : Internal diameter of the column

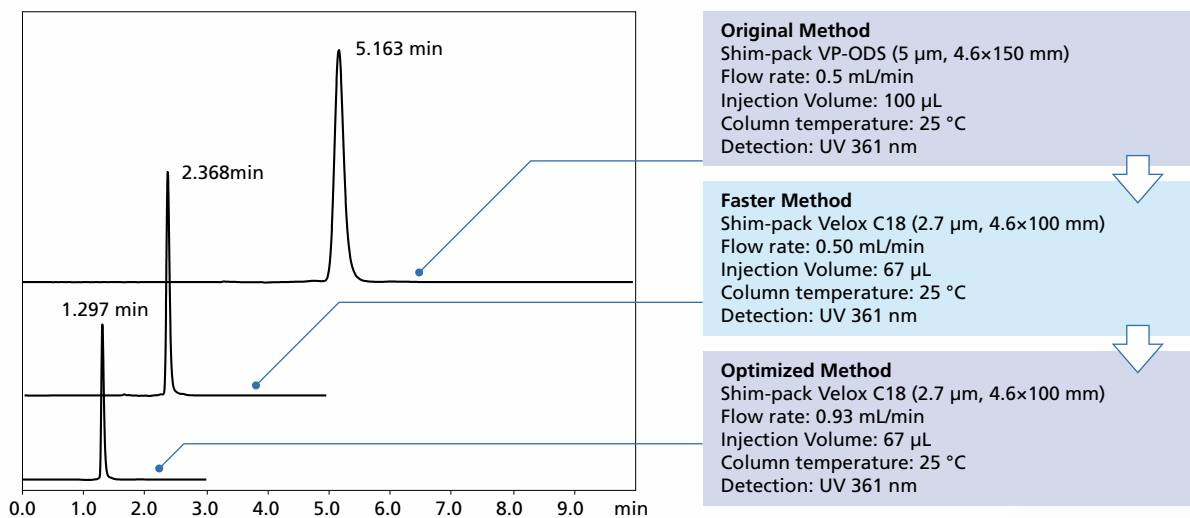

Column	L/dp	Flow rate (mL/min)	N	System suitability test result (Requirement: %RSD < 2.0 %)
VP-ODS (5 µm, 4.6×150 mm)	30,000	0.50	5,244	tR: 0.025 % Area: 0.175 % (n=6)
Velox C18 (2.7 µm, 4.6×100 mm)	37,037 (+23 %)	0.50	9,497 (+81 %)	tR: 0.035 % Area: 0.103 % (n=6)
		0.93	4,466 (-15 %)	tR: 0.084 % Area: 0.220 % (n=6)

Shim-pack Velox Biphenyl





Shim-pack Velox Biphenyl provides enhanced retention of aromatic compounds. It is useful for fast separations in bioanalytical applications due to the increased retention of early eluting analytes such as dipolar, unsaturated and conjugated analytes.

- Complementary selectivity to alkyl phases
- Enhanced separation of aromatic compounds
- Ideal for increasing sensitivity and selectivity in LC/MS(/MS) analysis

Separating the Structural Isomers

Even under the condition where 56 drugs of abuse and metabolites in human urine are quantitated within 10 minutes, two structural isomers, amobarbital and pentobarbital, which have been historically difficult to separate due to their similarity in chemical structures, could be relatively well resolved with shim-pack Velox Biphenyl column.

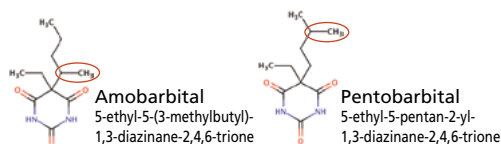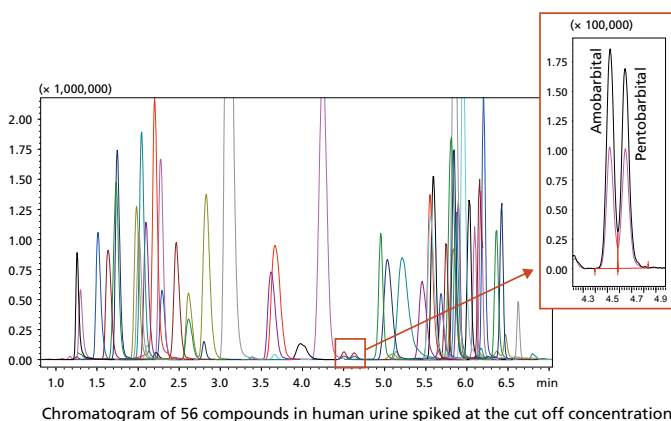

System: Nexera UHPLC System / LCMS-8050
Column: Shim-pack Velox Biphenyl 2.7 μ m, 2.1 mm \times 100 mm (PN: 227-32015-03)

Column Temp.: 30 $^{\circ}$ C

Flow Rate: 0.5 mL/min

Mobile Phase A: 0.15 mM ammonium fluoride in water

Mobile Phase B: Methanol

Gradient: 20 % B (0 min) \rightarrow 48 % B (1.5 min) \rightarrow 53 % B (4 min)


\rightarrow 100 % B (6 min - 7.5 min) \rightarrow 20 % B (7.51 min - 9.5 min)

Sample preparation:

Enzymatically hydrolyzed human urine was spiked with target compounds between 10 - 1000 % of the required cut off concentration.

Samples were subsequently diluted 5x with 0.1 % formic acid.

Shim-pack Velox PFPP





Shim-pack Velox PFPP (Pentafluorophenylpropyl) provides an alternative selectivity to C18 columns and is suitable for the analysis of halogenated compounds, positional isomers and charged bases.

- Alternative selectivity to C18 columns
- Suitable for positional isomers and halogenated compounds
- Offers increased retention for charged bases

Good Separation of Cis / Trans Stilbene

Cis and trans isomers of stilbene that are difficult to resolve with an ODS column due to their similarity in hydrophobicity can be well separated with Shim-pack Velox PFPP column.

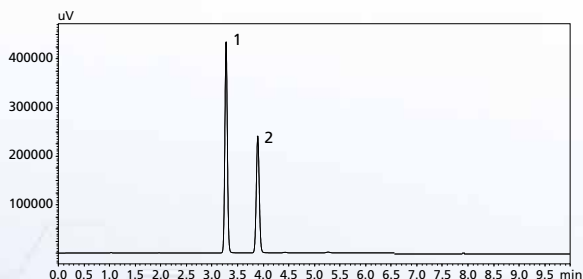

LC Conditions

Column: Shim-pack Velox PFPP, 2.7 μ m, 3.0 \times 100 mm (PN: 227-32022-04)

Column Temp.: 40 $^{\circ}$ C

Flow Rate : 0.4 mL/min

Mobile Phase : Methanol/Water = 9/1

Detection : UV 254 nm

Sample: 1. *cis*-Stilbene, 2. *trans*-Stilbene

Injection Volume : 1 μ L

Shim-pack Velox HILIC



Hydrophilic interaction chromatography (HILIC) is an increasingly popular separation mode that can be used to improve the retention of challenging polar analytes. Shim-pack Velox HILIC using unbonded core shell particles is specifically designed for this application.



- Orthogonal selectivity to reversed phase chromatography
- Increased retention of polar analytes
- Increased MS sensitivity
- Direct compatibility with sample preparation eluates

Retention of Nucleosides

Nucleosides are polar molecules that are not well retained on reversed phase LC columns due to their hydrophilic nature. They are well retained and separated with Shim-pack Velox HILIC column.

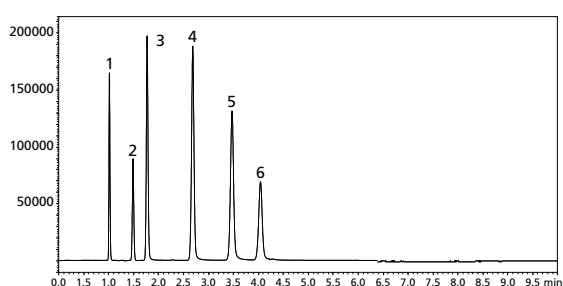

LC Conditions
 Column: Shim-pack Velox HILIC, 2.7 μ m, 3.0 \times 100 mm (PN: 227-32026-02)
 Column Temp.: 30 $^{\circ}$ C
 Flow Rate : 0.4 mL/min
 Mobile Phase : Acetonitrile/20mM AcONH₄aq.=9/1
 Detection : UV 254 nm
 Sample1. Toluene, 2. Uracil, 3. Uridine, 4. Adenosine, 5. Guanosine, 6. Cytidine
 Injection Volume : 1 μ L

Ordering Information

Shim-pack Velox 1.8 μ m Columns

Chemistry	SP-C18		C18		Biphenyl		PFPP		
	ID(mm)	2.1	3.0	2.1	3.0	2.1	3.0	2.1	3.0
30	227-32001-01	–	227-32007-01	–	227-32013-01	–	227-32019-01	–	–
50	227-32001-02	227-32002-01	227-32007-02	227-32008-01	227-32013-02	227-32014-01	227-32019-02	227-32020-01	–
100	227-32001-03	227-32002-02	227-32007-03	227-32008-02	227-32013-03	227-32014-02	227-32019-03	227-32020-02	–
150	227-32001-04	–	227-32007-04	–	227-32013-04	–	227-32019-04	–	–

Shim-pack Velox 2.7 μ m Columns

Chemistry	SP-C18			C18			Biphenyl			
	ID(mm)	2.1	3.0	4.6	2.1	3.0	4.6	2.1	3.0	4.6
30	227-32003-01	227-32004-01	227-32005-01	227-32009-01	227-32010-01	227-32011-01	227-32015-01	227-32016-01	227-32017-01	–
50	227-32003-02	227-32004-02	227-32005-02	227-32009-02	227-32010-02	227-32011-02	227-32015-02	227-32016-02	227-32017-02	–
100	227-32003-03	227-32004-03	227-32005-03	227-32009-03	227-32010-03	227-32011-03	227-32015-03	227-32016-03	227-32017-03	–
150	227-32003-04	227-32004-04	227-32005-04	227-32009-04	227-32010-04	227-32011-04	227-32015-04	227-32016-04	227-32017-04	–

Chemistry	PFPP			HILIC			
	ID(mm)	2.1	3.0	4.6	2.1	3.0	4.6
30	227-32021-01	227-32022-01	227-32023-01	227-32025-01	–	–	–
50	227-32021-02	227-32022-02	227-32023-02	227-32025-02	227-32026-01	227-32027-01	–
100	227-32021-03	227-32022-03	227-32023-03	227-32025-03	227-32026-02	227-32027-02	–
150	227-32021-04	227-32022-04	227-32023-04	227-32025-04	227-32026-03	227-32027-03	–

Ordering Information

Shim-pack Velox 5 μ m Columns

Chemistry	SP-C18	C18	Biphenyl	PFPP
Length(mm) \ ID(mm)	4.6			
50	227-32006-01	227-32012-01	227-32018-01	227-32024-01
100	227-32006-02	227-32012-02	227-32018-02	227-32024-02
150	227-32006-03	227-32012-03	227-32018-03	227-32024-03
250	227-32006-04	227-32012-04	227-32018-04	227-32024-04

Shim-pack Velox EXP Guard Column Cartridge (3 pk)

Type	UHPLC				2.7 μ m				
ID (mm)	SP-C18	C18	Biphenyl	PFPP	SP-C18	C18	Biphenyl	PFPP	HILIC
2.1	227-32028-01	227-32031-01	227-32034-01	227-32037-01	227-32029-01	227-32032-01	227-32035-01	227-32038-01	227-32040-01
3.0	227-32028-02	227-32031-02	227-32034-02	227-32037-02	227-32029-02	227-32032-02	227-32035-02	227-32038-02	227-32040-02
4.6	–	–	–	–	227-32029-03	227-32032-03	227-32035-03	227-32038-03	227-32040-03

Type	5 μ m			
ID (mm)	SP-C18	C18	Biphenyl	PFPP
4.6	227-32030-01	227-32033-01	227-32036-01	227-32039-01


*Shim-pack EXP Direct Connect Holder : 227-32041-01

Shim-pack Velox UHPLC Precolumn Filter (0.2 μ m)

Part No. 1 pack	227-32042-01
Part No. 5 pack	227-32042-02
Part No. 10 pack	227-32042-03


Shim-pack Velox EXP Guard Column

Free-turning architecture lets you change cartridges by hand without breaking inlet / outlet fluid connections — no tools needed. Guard column cartridges require Shim-pack EXP Direct Connect Holder (227-32041-01)

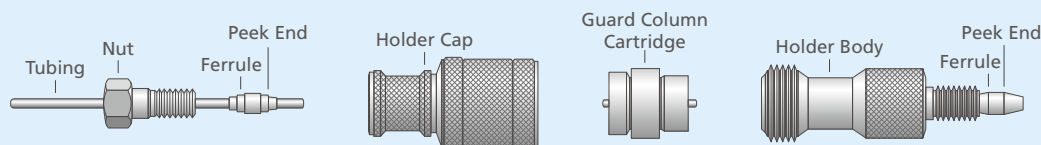

Shim-pack Velox UHPLC Precolumn Filter (0.2 μ m)

To minimize extra column volume and maximize UHPLC sample throughput with SPE, SLE, or other sample preparation techniques, pair 1.8 μ m Shim-pack Velox UHPLC columns with an Shim-pack Velox UHPLC Precolumn filter instead of a guard cartridge.



Shim-pack, Shim-pack Velox, CoreFocus logo and Nexera are trademarks of Shimadzu Corporation or its affiliated companies in Japan and/or other countries.



Shimadzu Corporation

www.shimadzu.com/an/

For Research Use Only. Not for use in diagnostic procedures.

This publication may contain references to products that are not available in your country. Please contact us to check the availability of these products in your country.

Company names, products/service names and logos used in this publication are trademarks and trade names of Shimadzu Corporation, its subsidiaries or its affiliates, whether or not they are used with trademark symbol "TM" or "®".

Third-party trademarks and trade names may be used in this publication to refer to either the entities or their products/services, whether or not they are used with trademark symbol "TM" or "®".

Shimadzu disclaims any proprietary interest in trademarks and trade names other than its own.

The contents of this publication are provided to you "as is" without warranty of any kind, and are subject to change without notice. Shimadzu does not assume any responsibility or liability for any damage, whether direct or indirect, relating to the use of this publication.