


InertSearch™ for GC

InertCap® Applications

Impurity in Ethanol

Data No. GA053-0000

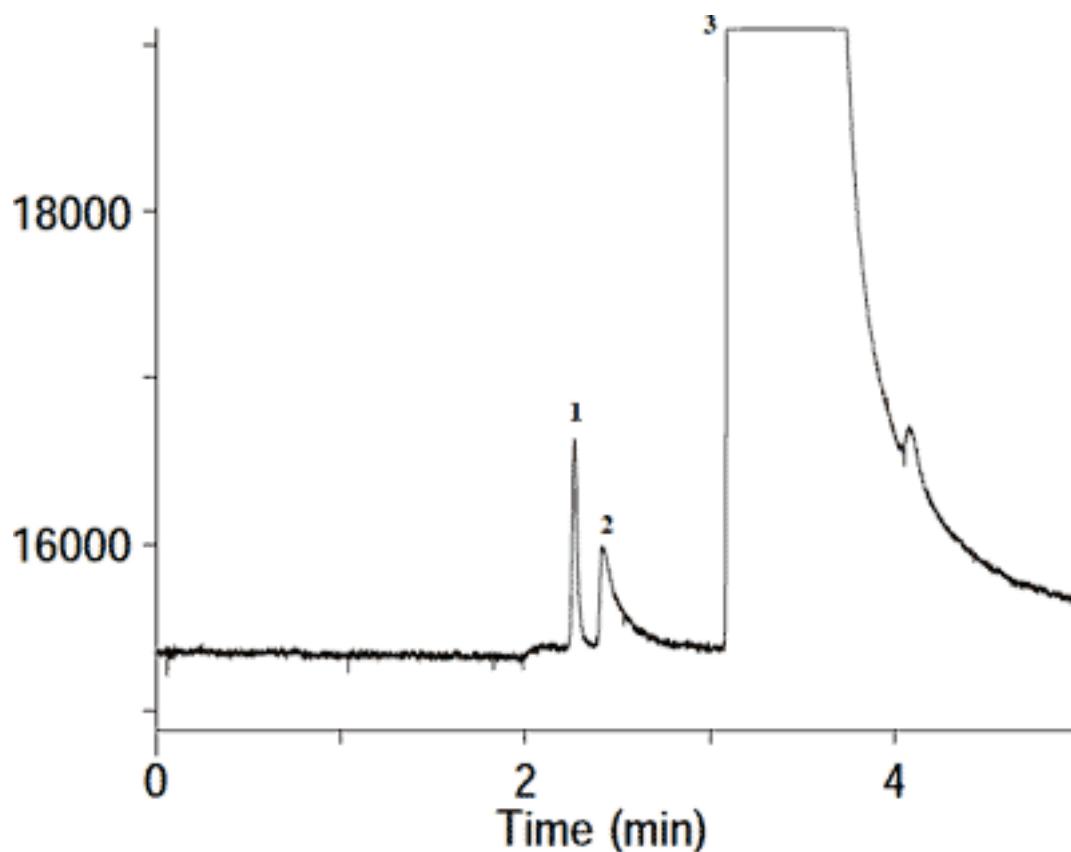

System : GC/FID
Column : InertCap 624
0.32mm I.D. x 30m df=1.80µm
Column Temp. : 40°C (12min) → 10°C/min → 240°C (10min)
Carrier Gas : He 60kPa
Injection : Split 1:20 1µL
Detection : FID

Solutes : 1. Acetaldehyde
2. Methanol
3. Ethanol