


Analysis of butter fat

HT5

Column part number	054661		
Phase	HT5	Carrier gas	H ₂ , 2 psi
Column	6 m x 0.53 mm x 0.1 μm	Detector	FID
Initial temperature	200°C, 0 min	Sensitivity	32 x 10 ⁻¹² AFS
Rate	10°C/min	Injection mode	On-column
Final temperature	370°C, 5 min		

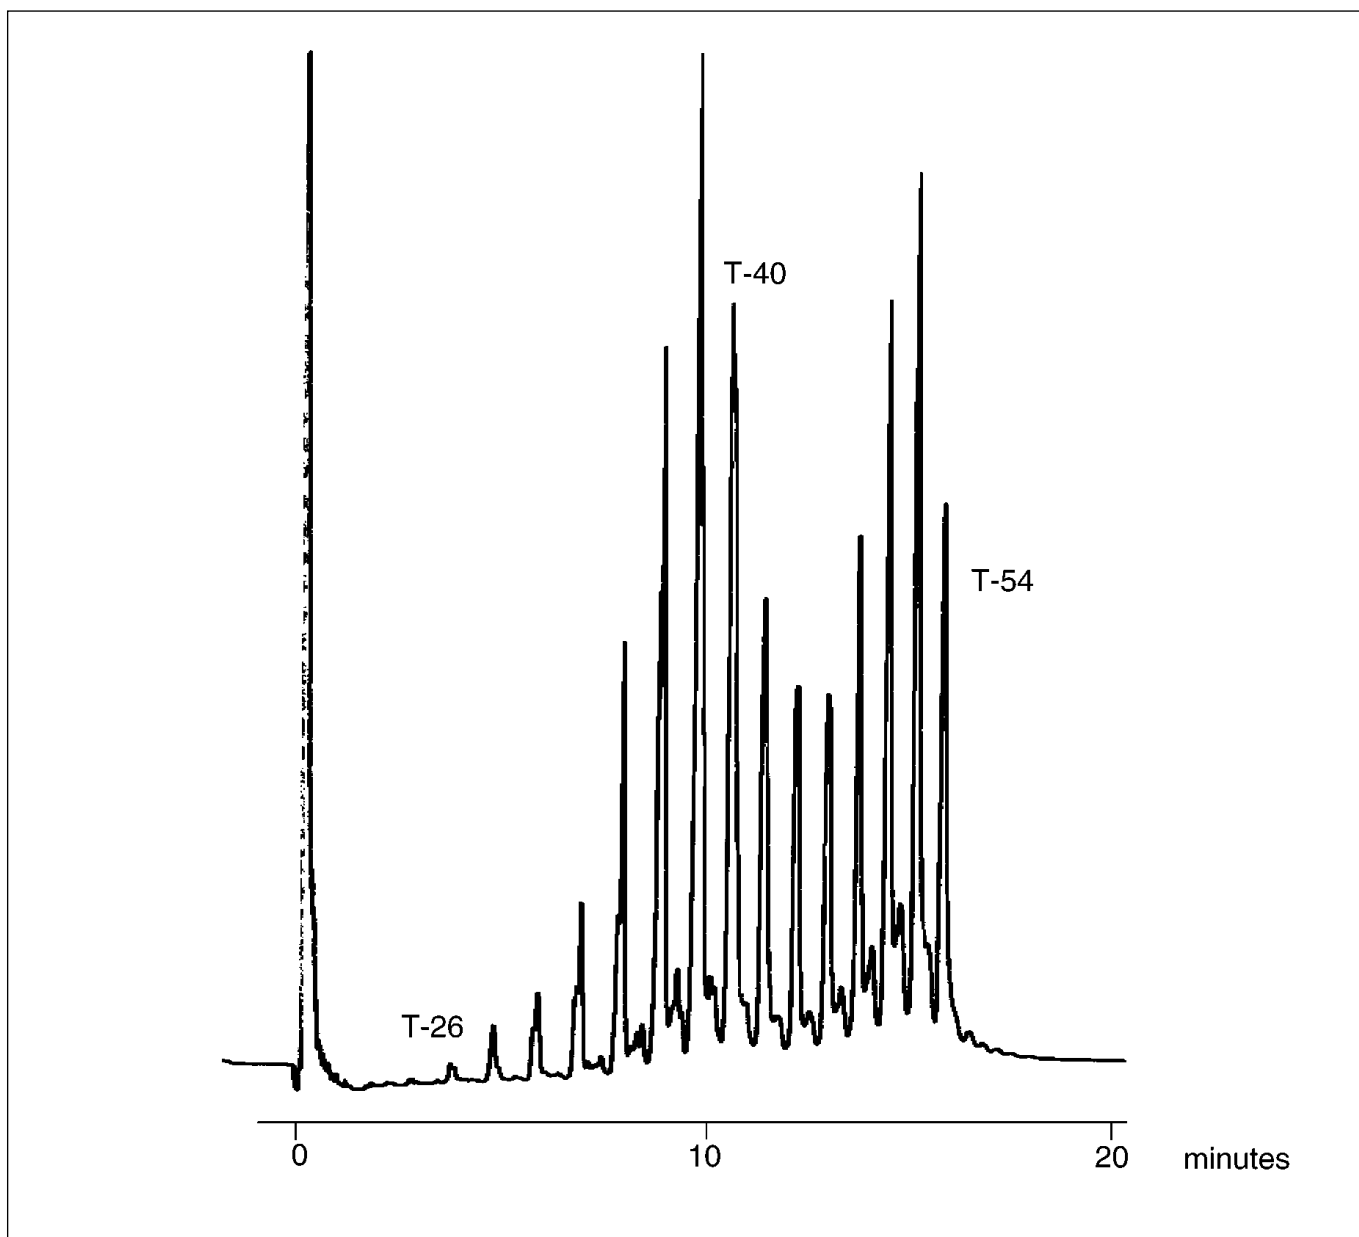

For more information visit www.trajanscimed.com or contact techsupport@trajanscimed.com