

Application News

No. M273

Gas Chromatograph Mass Spectrometry

Analysis of Short-Chain Fatty Acids in Biological Samples Using GC-MS

Short-chain fatty acids, such as acetic acid, are compounds that have been commonplace in our lives from long ago. While they are recently gaining attention as useful components within intestinal flora, they are also known as compounds that prove difficult to quantitatively analyze. Generally, quantitation at low concentrations is not possible by LC-MS since formic acid and acetic acid are used in the mobile phase. With GC-MS, which requires derivatization of hydroxyl groups, there is the problem where most short-chain fatty acids volatilize when drying moisture in samples, a process necessary in most derivatization processes.

In this research, we avoided this problem by using the condensing agent 4-(4,6-Dimethoxy-1,3,5-triazin-2-yl)-4-methylmorpholinium Chloride (DMT-MM), which induces condensation reactions between carboxylic acid and amines even in water or methanol, to derivatize short-chain fatty acids with an amine and then performed GC-MS analysis. We also evaluated the quantitative performance of the analysis system when analysis is performed using derivatization.

T. Sakai

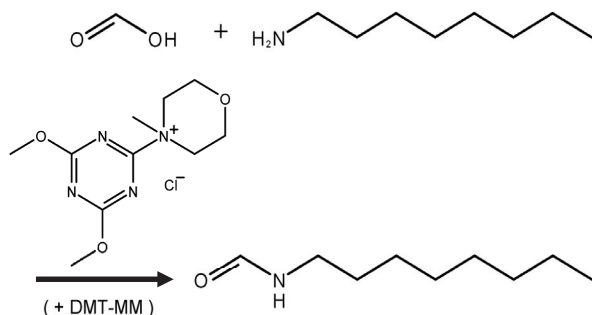


Fig. 1 Condensation Reaction Between Formic Acid and n-Octyl Amine

Sample

Pretreatment was performed on human standard plasma (Kohjin Bio Co., Ltd.: Human Plasma Pooled - EDTA-2Na (12271450)) and the concentration of each fatty acid was measured using the standard addition method.

50 μ L of sample

↓
Add 10 μ L of short-chain fatty acid mixed aqueous solution to obtain a final concentration of 0 to 100 μ mol/L.

↓
Add acetic acid-d₄ aqueous solution to obtain a final concentration of 10 μ mol/L.

↓
Add 250 μ L of methanol. (deproteinization)

↓
Perform high-speed shaking for 30 seconds and then centrifuge for 3 minutes at 25 °C and 16,000 G.

↓
Collect 180 μ L of supernatant.

↓
Add 20 μ L of methanol solution that contains 100 mmol/L of both DMT-MM and n-octyl amine.

↓
Leave standing at room temperature for 9 hours and then analyze.

Fig. 2 Pretreatment of Human Standard Plasma

Analysis Conditions

Table 1 lists the analysis conditions.

Table 1 Measurement Conditions

GC	
Column	: BPX-5 (30 m \times 0.25 mm I.D. 0.25 μ m)
Carrier Gas	: He
Injection Port Temp.	: 250 °C
Carrier Gas Control	: Linear Velocity (39.0 cm/sec)
Injection Mode	: Split (30:1)
Oven Temp.	: 60 °C (2 min) \rightarrow 15 °C/min \rightarrow 330 °C (5 min)
MS	
Ion Source Temp.	: 200 °C
Interface Temp.	: 280 °C
Measurement Mode	: MRM
Loop Time	: 0.3 sec

Results

The calibration curves for the fatty acid derivatives all showed good linearity and we were able to measure the concentration of each type of short-chain fatty acid in the human standard plasma (Table 2).

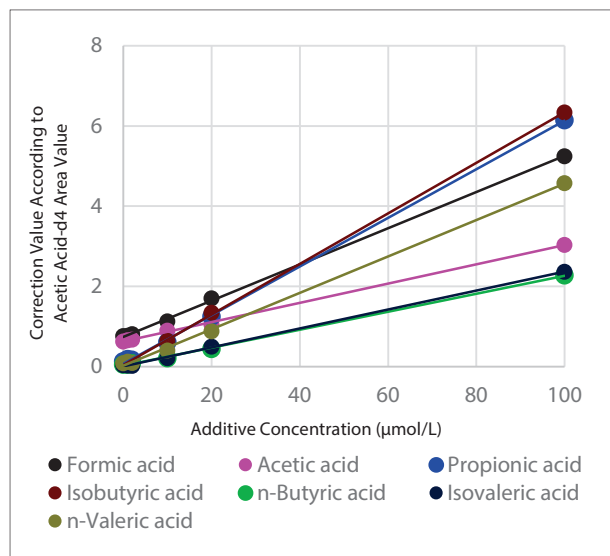


Fig. 3 Fatty Acid Calibration Curves

Table 2 Calibration Curve Linearity and Concentration in Human Standard Plasma

Compound Name	Linearity of Calibration Curve (R ² Value)	Concentration in Plasma (µmol/L)
Formic acid	0.9994	115.64
Acetic acid	0.9990	184.36
Propionic acid	0.9996	8.02
Isobutyric acid	0.9997	3.97
n-Butyric acid	0.9991	5.89
Isovaleric acid	0.9992	0.82
n-Valeric acid	0.9991	3.25

Conclusion

We were able to quantitatively analyze seven types of short-chain fatty acids, namely formic acid, acetic acid, propionic acid, butyric acid, isobutyric acid, valeric acid, and isovaleric acid, in a biological sample by GC-MS, by performing the following:

- Performing derivatization with amines using DMT-MM
- Normalizing area values using acetic acid-d4 as the internal standard

References:

The information in this article presents an experiment and verification performed by Shimadzu, based on a technique described in "The TRC News No. 115 (May 2012)" published by Toray Research Center, Inc.

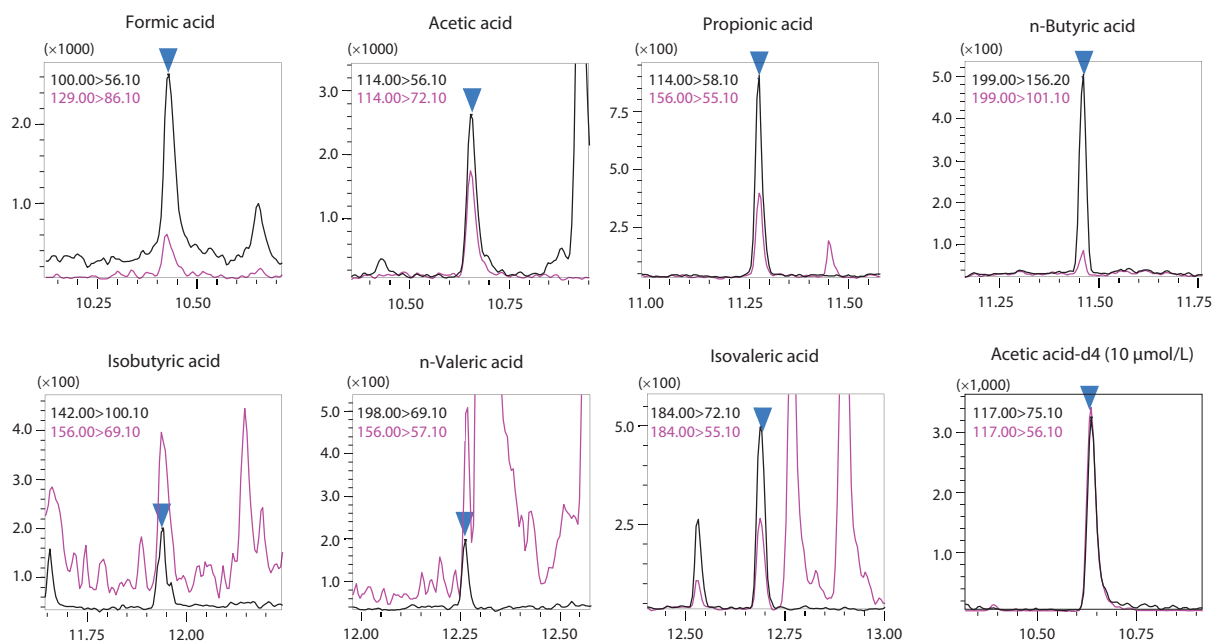


Fig. 4 MRM Chromatograms of Sample Spiked at 1 µmol/L

Note: The product described in this document has not been approved or certified as a medical device under the Pharmaceutical and Medical Device Act of Japan. It cannot be used for the purpose of medical examination and treatment or related procedures.

First Edition: Apr. 2017



For Research Use Only. Not for use in diagnostic procedure.

This publication may contain references to products that are not available in your country. Please contact us to check the availability of these products in your country.

The content of this publication shall not be reproduced, altered or sold for any commercial purpose without the written approval of Shimadzu. Company names, product/service names and logos used in this publication are trademarks and trade names of Shimadzu Corporation or its affiliates, whether or not they are used with trademark symbol "TM" or "®". Third-party trademarks and trade names may be used in this publication to refer to either the entities or their products/services. Shimadzu disclaims any proprietary interest in trademarks and trade names other than its own.

The information contained herein is provided to you "as is" without warranty of any kind including without limitation warranties as to its accuracy or completeness. Shimadzu does not assume any responsibility or liability for any damage, whether direct or indirect, relating to the use of this publication. This publication is based upon the information available to Shimadzu on or before the date of publication, and subject to change without notice.

Shimadzu Corporation

www.shimadzu.com/an/